

DECLARATION OF BLOOD PRESSURE MEASURING DEVICE EQUIVALENCE

A SIGNED COPY WILL BE POSTED ON THE www.dableducational.org WEBSITE

SECTION A - Please complete all items.

I **Bill Huang,** a Director of **AVITA Corporation,**
Name of a Company Director Company name

hereby state that there are no differences that will affect blood pressure measuring accuracy between the

Maker^a	BEURER GmbH	Address	Soeflinger Strasse 218, 89077 Ulm, Germany
Manufacturer^b	AVITA Corporation	Address	9F, NO.78, SEC.1, KWANG-FU RD. , SAN –Chung District, New Taipei City 24158 Taiwan R.O.C.
Brand^c	Beurer	Model^d	BM 51

Blood pressure measuring device for which validation is claimed. If alternative model names are used, include all.

blood pressure measuring device and the validated blood pressure measuring device

Maker^a	AVITA Corporation	Address	9F, NO.78, SEC.1, KWANG-FU RD. , SAN –Chung District, New Taipei City 24158 Taiwan R.O.C.
Manufacturer^b	AVITA Corporation	Address	9F, NO.78, SEC.1, KWANG-FU RD. , SAN –Chung District, New Taipei City 24158 Taiwan R.O.C.
Brand^c	AVITA	Model^d	BPM64

Existing validated blood pressure measuring device.

which has previously passed the ESH-2010 protocol, the results of which were published as follows:

Kang Y.Y., Chen Q., Liu C.Y., Li Y. and Wang J.G. Validation of the AVITA BPM64 upper-arm blood pressure monitor for home blood pressure monitoring according to the European Society of Hypertension International Protocol revision 2010.

Full reference

The only differences between the devices involve the following components:

Tick one box for each item 1–18.

Part I	1	Algorithm for Oscillometric Measurements	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	N/A ^e <input type="checkbox"/>
	2	Algorithm for Auscultatory Measurements	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^f <input checked="" type="checkbox"/>
	3	Artefact/Error Detection	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	4	Microphone(s)	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^f <input checked="" type="checkbox"/>
	5	Pressure Transducer	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	6	Cuffs or Bladders	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	7	Inflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	8	Deflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
Part II	9	Model Name or Number	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	10	Casing	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	11	Display	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	12	Carrying/Mounting Facilities	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	13	Software other than Algorithm	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	14	Memory Capacity/Number of stored measurements	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	15	Printing Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^g <input checked="" type="checkbox"/>
	16	Communication Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^g <input checked="" type="checkbox"/>
	17	Power Supply	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	18	Other Facilities	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	N/A ^g <input type="checkbox"/>

An explanation of each item ticked "Yes" must be included in Section B or on a separate sheet.

- Notes:
- a Provide the name and address of the actual maker of the device.
 - b Provide the name and address of the legal manufacturer of the device, even if it is the same as that of the maker.
 - c Provide the name of the brand under which it is sold, even if it is the same as that of the manufacturer or maker.
 - d Provide the model name. If alternative or internal model names are used, include all. Each device must be uniquely identifiable.
 - e Only tick N/A (Not Applicable) if neither device measures blood pressure using the oscillometric method.
 - f Only tick N/A (Not Applicable) if neither device measures blood pressure using the auscultatory method.
 - g Only tick N/A (Not Applicable) if neither device provides printing, communication or other facilities, as appropriate.

SECTION B An explanation for each item, 1 to 18, ticked "Yes" in Section A must be provided here or in an attached document. All differences between the devices must be described.

- 9) The model name is different. for new device and validated device is BPM64
10) The designs of the case are different.
11) The size and displayed data are different.
12) Carrying/Mounting Facilities are different.
14) has 2*100 memories
17) New model use AA*1.5V batteries or AC adaptor 100 – 240 V, 50 – 60 Hz, 0.5 A max

SECTION C Please check that the following are included with the application

- A manual for the validated device
A manual for the device for which equivalence is being sought
Completed DET9 Form
An image of the device for which equivalence is being sought
An image of the screen layout of validated device*
An image of the screen layout of the device for which equivalence is being sought*

* Screen layouts shown complete, and without obscuring labels or lines, in manuals need not be included separately.

SECTION D Complete all items, bar signatures and seal, online and print. Sign and seal it then send the original to our address below. Please email a signed copy of this form, together with the manuals and images for both devices, to info@dableducational.org.

Signature of Director _____

Company Stamp/Seal

Name [Handwritten Signature] 8/19.2019

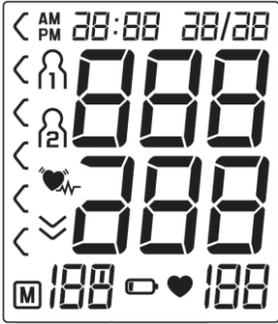
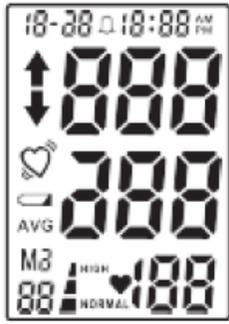
Date

Signature of Witness _____

Name [Handwritten Signature: Jonathan Chen] 2019.8.19.

Address 9F, NO.78, SEC.1, KWANG-FU RD. , SAN -Chung District, New Taipei City 24158 Taiwan R.O.C.

Comparison of the Beurer BM51 with the AViTA BPM64

Devices – Item 9	Beurer BM51	AViTA BPM64
Pictures		
Display Image		
Validation		ESH 2010
Category	Upper Arm Type Blood Pressure Monitor	Upper Arm Type Blood Pressure Monitor
Casing – Item 10	<p><i>Dimensions</i> approx. 138 mm x 103 mm x 44 mm (W * H *D)</p> <p><i>Ports</i> Cuff Port DC Jack Port</p> <p><i>Features</i> ABS plastic part Printing</p>	<p><i>Dimensions</i> approx. 113mm x 140mm x 57mm (W x H x D)</p> <p><i>Ports</i> Cuff Port</p> <p><i>Features</i> ABS Plastic part Printing</p>
Display – Item 11	LCD	LCD

Carrying/Mounting Facilities – Item 12	Storage Box	<i>Storage Box</i>
Software other than Algorithm – Item 13	N/A	<i>N/A</i>
Memory Capacity Item 14	2*100 times with date and time	1*90 times with date and time
Printing Facilities Item 15	Artwork logo, gift box and manual is different from AVITA BPM64 for different functions	Artwork logo, gift box and manual is different <i>for different functions</i>
Communication Facilities – Item 16	N/A	<i>N/A</i>
Power Supply Item 17	4 * AA Batteries AC adaptor Input: 100 – 240 V, 50 – 60 Hz, 0.5 A max Output: 6V DC, 600 mA	4 * AA Batteries
Other differences	<i>Accuracy</i> Blood Pressure Accuracy ± 3 mmHg Pulse Accuracy $\pm 5\%$	<i>Accuracy</i> Blood Pressure Accuracy ± 3 mmHg Pulse Accuracy $\pm 4\%$
Same Criteria	<p>Measurement</p> <p><i>Method</i> Oscillometri</p> <p><i>Ranges</i> Cuff pressure 0–300 mmHg, systolic 60–255 mmHg, diastolic 40–200 mmHg,</p> <p><i>Inflation</i> Automatic inflation by internal pump</p> <p><i>Deflation</i> Automatic speed deflation system</p> <p><i>Cuffs (Please state sizes and materials used)</i> approx. 585 X 178 cm Bladder dimension: 230 X 125mm</p>	<p>Measurement</p> <p><i>Method</i> Oscillometri</p> <p><i>Ranges</i> Cuff pressure 0–300 mmHg, systolic 60–255 mmHg, diastolic 40–200 mmHg,</p> <p><i>Inflation</i> Automatic inflation by internal pump</p> <p><i>Deflation</i> Automatic speed deflation system</p> <p><i>Cuffs (Please state sizes and materials used)</i> approx. 580 X 150 cm Bladder dimension: 230 X 125mm</p>

	<p><i>Sensors</i> US-9111-006-S</p> <p><i>Measurement Records</i> 2*100 times with date and time</p> <p><i>Measurements other than Blood Pressure</i> Pulse rate</p> <p>Buttons/Switches <i>Power</i> START/POWER Button (on / off)</p> <p><i>Measurement Records</i> Memory Recall Button - MEM</p> <p><i>Function</i> Date and Time Set Button – SET “-/+” function buttons - select the relevant value</p> <p><i>Analysis</i> N/A</p> <p><i>Event Marking</i> N/A</p> <p><i>Communication</i> N/A</p> <p>Display/Symbols/Indicators <i>Preparation</i> N/A</p> <p><i>Measurement Procedure</i> Inflation symbol Deflation symbol Heartbeat symbol during deflation Irregular Heartbeat symbol</p> <p><i>Post Measurement</i></p>	<p><i>Sensors</i> US-9111-006-S</p> <p><i>Measurement Records</i> 1*90 times with date and time</p> <p><i>Measurements other than Blood Pressure</i> Pulse rate</p> <p>Buttons/Switches <i>Power</i> START/POWER Button (on / off)</p> <p><i>Measurement Records</i> Memory Recall Button - MEM</p> <p><i>Function</i> Date and Time Set Button – SET Mode (Alarm) Button - Mode</p> <p><i>Analysis</i> N/A</p> <p><i>Event Marking</i> N/A</p> <p><i>Communication</i> N/A</p> <p>Display/Symbols/Indicators <i>Preparation</i> N/A</p> <p><i>Measurement Procedure</i> Inflation symbol Deflation symbol Heartbeat symbol during deflation Irregular Heartbeat symbol</p> <p><i>Post Measurement</i></p>
--	---	--

	<p>Systolic blood pressure Diastolic blood pressure Pulse rate WHO indicator</p> <p><i>Measurement Records</i> Memory recall number</p> <p><i>Date and Time</i> Date and Time</p> <p><i>Power</i> Low Battery detection symbol</p> <p><i>Function</i> Average</p> <p><i>Communication</i> N/A</p> <p><i>Features</i> N/A</p> <p><i>Not described</i> N/A</p> <p>Algorithms <i>Averages and Differences</i> Average of all measurement Average morning values of the last seven days measurements between 5:00AM and 9:00AM Average evening values of the last seven days measurements between 6:00PM and 8:00PM</p> <p><i>Diagnostic</i> N/A</p> <p><i>Functions</i> N/A</p> <p><i>Communication</i> N/A</p>	<p>Systolic blood pressure Diastolic blood pressure Pulse rate WHO indicator</p> <p><i>Measurement Records</i> Memory recall number</p> <p><i>Date and Time</i> Date and Time</p> <p><i>Power</i> Low Battery detection symbol</p> <p><i>Function</i> Average Alarm</p> <p><i>Communication</i> N/A</p> <p><i>Features</i> N/A</p> <p><i>Not described</i></p> <p>Algorithms <i>Averages and Differences</i> Average of the last 3 measurements</p> <p><i>Diagnostic</i> N/A</p> <p><i>Functions</i> N/A</p> <p><i>Communication</i> N/A</p>
<p>Comparable Criteria</p>		

Comments		
Recommendation	Recommended	
Date	25th September 2020	