

DECLARATION OF BLOOD PRESSURE MEASURING DEVICE EQUIVALENCE 2013

A SIGNED COPY WILL BE POSTED ON THE www.dableducational.org WEBSITE

SECTION A - Please complete all items.

I Liu Yi, a Director of Andon Health Co.,Ltd.,
Name of a Company Director Company name

hereby state that there are no differences that will affect blood pressure measuring accuracy between the

Maker ^a	CITIZEN	Address	6-1-12 Tanashi-cho, Nishi-Tokyo-shi, Tokyo 188-8511, Japan
Manufacturer ^b	Andon	Address	Andon Health Co., Ltd. No.3 Jin Ping Street, Ya An Road, Nankai District, Tianjin 300190, China
Brand ^c	CITIZEN	Model ^d	CHU304

Blood pressure measuring device for which validation is claimed. If alternative model names are used, include all.

blood pressure measuring device and the validated blood pressure measuring device

Maker ^a	Andon	Address	Andon Health Co., Ltd. No.3 Jin Ping Street, Ya An Road, Nankai District, Tianjin 300190, China
Manufacturer ^b	Andon	Address	Andon Health Co., Ltd. No.3 Jin Ping Street, Ya An Road, Nankai District, Tianjin 300190, China
Brand ^c	Andon	Model ^d	KD-5915

Existing validated blood pressure measuring device.

which has previously passed the ESH2002 protocol, the results of which were published as follows:

Huang QF, Wang J, Sheng CS, Zhang NN, Li Y, Wang JG. Validation of the ANDON KD-5915 blood pressure monitor for home blood pressure monitoring according to the European Society of Hypertension International Protocol. Blood Press Monit 2010;15(4)

Full reference

The only differences between the devices involve the following components:

Tick one box for each item 1-18.

Part I	1	Algorithm for Oscillometric Measurements	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	N/A ^e <input type="checkbox"/>
	2	Algorithm for Auscultatory Measurements	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^f <input checked="" type="checkbox"/>
	3	Artefact/Error Detection	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	4	Microphone(s)	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^f <input checked="" type="checkbox"/>
	5	Pressure Transducer	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	6	Cuffs or Bladders	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	7	Inflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	8	Deflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
Part II	9	Model Name or Number	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	10	Casing	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	11	Display	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	12	Carrying/Mounting Facilities	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	13	Software other than Algorithm	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	14	Memory Capacity/Number of stored measurements	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	15	Printing Facilities	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	N/A ^g <input checked="" type="checkbox"/>
	16	Communication Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^g <input checked="" type="checkbox"/>
	17	Power Supply	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	18	Other Facilities	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	N/A ^g <input type="checkbox"/>

An explanation of each item ticked "Yes" must be included in Section B or on a separate sheet.

- Notes:
- a Provide the name and address of the actual maker of the device.
 - b Provide the name and address of the legal manufacturer of the device, even if it is the same as that of the maker.
 - c Provide the name of the brand under which it is sold, even if it is the same as that of the manufacturer or maker.
 - d Provide the model name; if alternative or internal model names are used, include all. Each device must be uniquely identifiable.
 - e Only tick N/A (Not Applicable) if neither device measures blood pressure using the oscillometric method.
 - f Only tick N/A (Not Applicable) if neither device measures blood pressure using the auscultatory method.
 - g Only tick N/A (Not Applicable) if neither device provides printing, communication or other facilities, as appropriate.

SECTION B An explanation for each item, 1 to 18, ticked "Yes" in Section A must be provided here or in an attached document. All differences between the devices must be described.

- (9)The model number is changed to CITIZEN CHU304 from ANDON KD-5915;
(10) They have the same botton but in the different position;
(11) No symbol for "find an error,please re-inflate";
(13)The average reading function is added(latest 3 readings in the memory);
(14) Stores 99 readings instead of 60 readings;
(18)No voice function;

SECTION C Please check that the following are included with the application

- A manual for the validated device
A manual for the device for which equivalence is being sought
An image of the validated device
An image of the device for which equivalence is being sought
An image of the screen layout of validated device*
An image of the screen layout of the device for which equivalence is being sought*
* Screen layouts shown complete, and without obscuring labels or lines, in manuals need not be included separately.

SECTION D Complete all items, bar signatures and seal, online and print. Sign and seal it then send the original to our address below. Please email a signed copy of this form, together with the manuals and images for both devices, to info@dableducational.org.

Signature of Director Liu Yi

Company Stamp/Seal

Name Liu Yi

Date 22 Dec. 2014



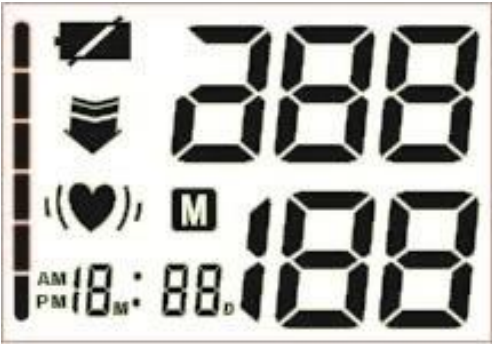

Signature of Witness Zhang Fei

Name Zhang Fei

Address Andon Health Co.,Ltd.No.3 Jin Ping Street,Ya An Road,Nankai District,Tianjin 300190,China



Comparison of the Andon KD-5915 with the Citizen CHU304

Devices	Citizen CHU304 (Device 2)	Andon KD-5915 (Device 1)
Pictures		
Display		
Validation		ESH 2002
Device 1 Criteria		<p><i>Memory</i> 60 Readings</p> <p><i>Voice Function</i> Yes</p> <p><i>Cuff Pressure</i> 0-295mmHg</p> <p><i>Average Reading</i> No</p>

		<p><i>Measurement Range</i> SBP 60-280 mmHg DBP 30-199 mmHg</p> <p><i>Dimension</i> Approximately 156mm x 101mm x 57mm</p> <p><i>Weight</i> Approximately 280g (Excluding batteries)</p>
<p>Device 2 Criteria</p>	<p><i>Memory</i> 99 Readings</p> <p><i>Voice Function</i> No</p> <p><i>Cuff Pressure</i> 0-300mmHg</p> <p><i>Average Reading</i> Yes</p> <p><i>Measurement Range</i> SBP 60-260 mmHg DBP 40-199 mmHg</p> <p><i>Dimension</i> Approximately 138mm x 54mm x 95mm</p> <p><i>Weight</i> Approximately 211g (Excluding batteries)</p>	
<p>Same Criteria</p>	<p><i>Measurement</i> <i>Accuracy</i> BP Accuracy ±3mmHg Pulse accuracy ±5mmHg</p>	<p><i>Measurement</i> <i>Accuracy</i> BP Accuracy ±3mmHg Pulse accuracy ±5mmHg</p>

	<p><i>Method</i> Oscillometric Pulse Rate Range 40-180 pulse/min</p> <p><i>Inflation</i> Automatic inflation by internal pump</p> <p><i>Deflation</i> Automatic speed deflation system</p> <p><i>Cuffs</i> 22cm-30cm Upper Arm Location</p> <p><i>Sensors</i> KD-2107-006G or KD-2107-006GR</p> <p>Display/Symbols/Indicators <i>Power</i> 4 AA Batteries</p> <p>Casing <i>Display</i> LCD</p>	<p><i>Method</i> Oscillometric Pulse Rate Range 40-180 pulse/min</p> <p><i>Inflation</i> Automatic inflation by internal pump</p> <p><i>Deflation</i> Automatic speed deflation system</p> <p><i>Cuffs</i> 22cm-30cm Upper Arm Location</p> <p><i>Sensors</i> KD-2107-006G or KD-2107-006GR</p> <p>Display/Symbols/Indicators <i>Power</i> 4 AA Batteries</p> <p>Casing <i>Display</i> LCD</p>
Comparable Criteria		
Device 2 Criteria		

Recommendation	<i>Recommended</i>
Date	27 January 2015