


Progress on the development of the MediWatch ambulatory blood pressure monitor and related devices

Blood Pressure Monitoring 2004, 14:327

The authors would like to make the following amendment to their article referenced below [1].

On page 151 of the article, the cross-section of the artificial wrist in Figure 3 is incorrect. This irregularity is corrected in the replacement figure below.

Fig. 3

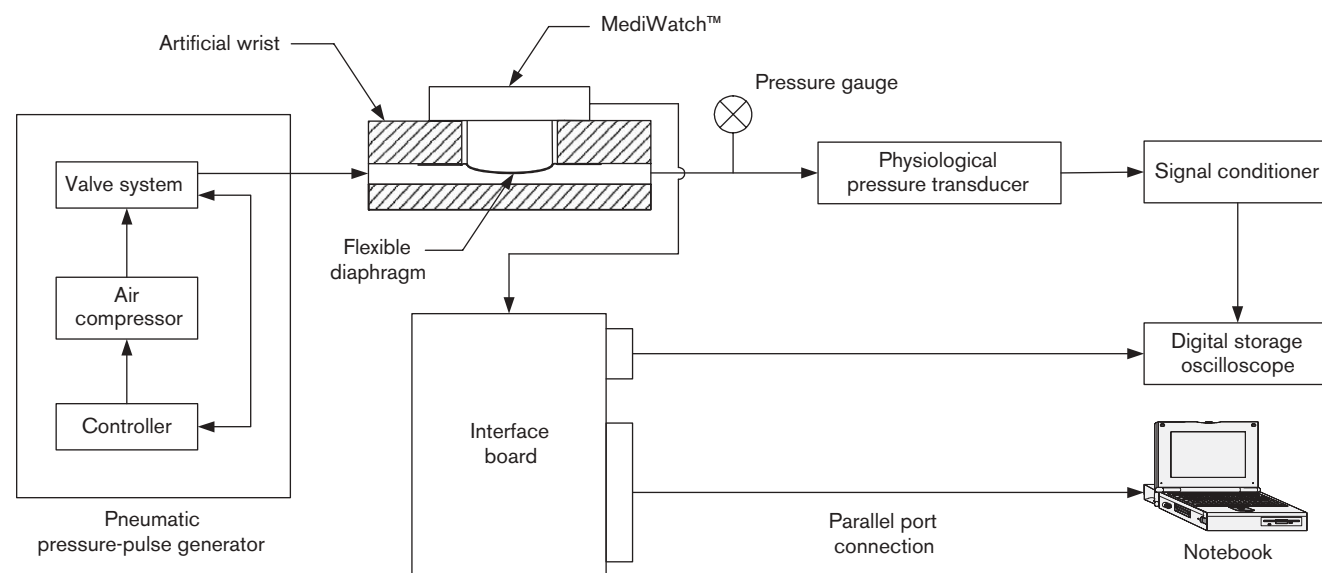

Setup for evaluation of the MediWatch prototype against simulated pressure waveforms.

References

- 1 Ng F-G, Ting C-M, Yeo J-H, Sim K-W, Chau N-H, *et al.* Progress on the development of the MediWatch ambulatory blood pressure monitor and related devices. *Blood Press Monit* 2004; **9**:149–165.